
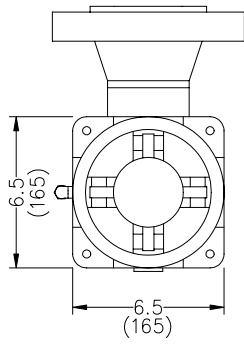
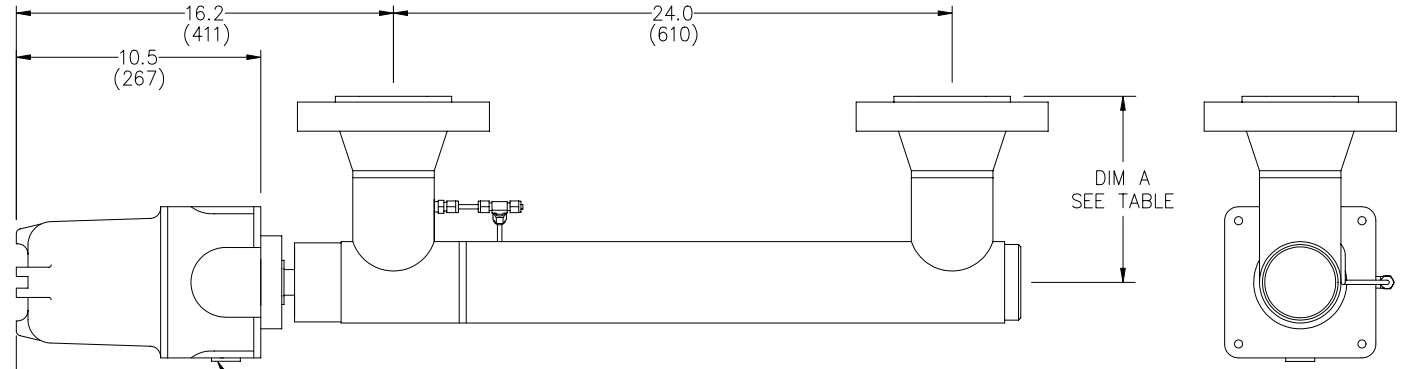


REV	DATE	ECO	COMMENTS
A	06/04/03	169	ADD METRIC UNITS
B	12/04/03	178	REMOVE 1500 FLANGE

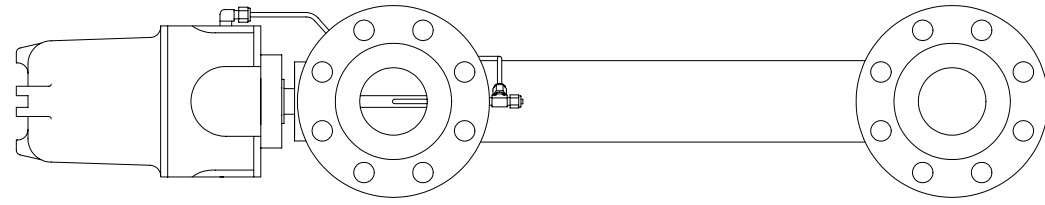


18 (457)
RECOMMENDED MINIMUM CLEARANCE FOR ACCESS

0.75-14 NPT REDUCING BUSHING (SUPPLIED)

NOTES:
1. ALL DIMENSIONS GIVEN IN INCHES
MILLIMETER DIMENSIONS SHOWN IN ()

FLANGE SIZE	DIMENSION "A"	WEIGHT	
		(LBS)	(KG)
ANSI 150	7.26 (184)	78	35
ANSI 300	7.63 (194)	91	41
ANSI 600	8.01 (203)	91	41
ANSI 900	8.76 (223)	113	51

 PHASE DYNAMICS, INC RICHARDSON, TEXAS	
TITLE INSTALLATION, 3 INCH U CONFIG RAISED FACE FLANGES	
SIZE	DWG NO. 0070-00155-000 DATE 06/19/99
REV	B © PHASE DYNAMICS, INC.